

References

- 1. Yaron, M., et al. An Innovative Atraumatic Uterine Cervical Traction Device: A Randomized Trial. Poster presented at: European Society of Contraception and Reproductive Health. Ghent Belgium, May 2022.a
- 2. Aspivix data on file.

Brief Statement

See Instructions for Use for detailed information regarding directions for use and device operationss, indications, contraindications, warnings, precautions, and potential adverse events. For further information, contact Aspivix at contact@aspivix.com and/or consult the Aspivix website at www.aspivix.com.



eifu.aspivix.com +800 135 79 135

About Aspivix

We're a medical device start-up from Switzerland. A nimble team of engineers, scientists, gynecologists and seasoned medical technology experts fully devoted to women's healthcare. Our vision at Aspivix is to make Gynecology. Now modern.

ASPIVIX SA

Global Headquarters Chemin du Closel 5 1020 – Renens Switzerland



Visit Us


Copyrights ©2022, Aspivix SA. All Rights Reserved. www.aspivix.com

P03-551-001 Rev A ©2022 Aspivix SA. Specifications are subject to change without prior notice. Aspivix, and Carevix are trademarks or registered trademarks of Aspivix SA and/or its subsidiaries. Licensed material is being used for illustrative purposes only. Any person depicted in the licensed material is a model.



How Carevix™ Works

Components

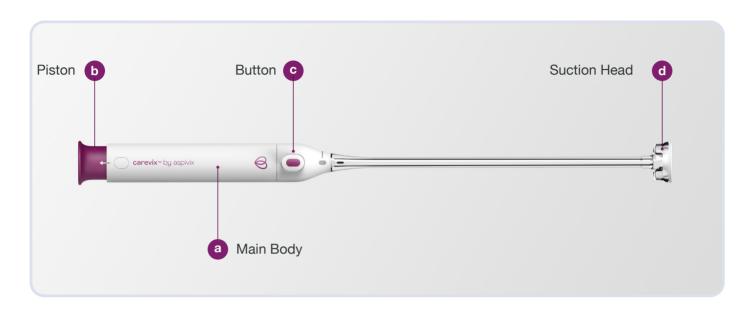

Assembling it



Connect the Suction Head to the Main Body.

Align the connecting marks found on the Suction Head and Main Body Rotate only the Main Body clockwise until it stops and the thin mark on the Main Body is aligned with the thick mark on the Suction Head.

Using Carevix™ - 3 Easy Steps




Pull the Piston to generate the vacuum and rotate to lock it.

Place the Suction Head on the cervix and press the Button downwards to deliver the vacuum.

Press the Button upwards to release the cervix.

During a clinical study, 100 patients were involved to measure pain experienced during IUD procedures.

Bleeding Results - All Women

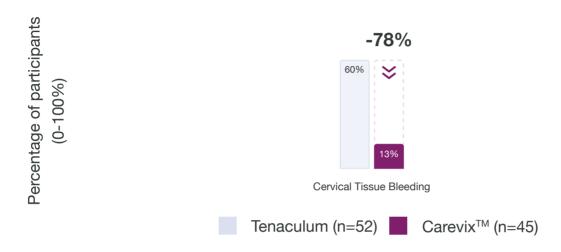

Cervical tissue bleeding frequency is significantly reduced (78% less frequent with Carevix™).


According to ASPIVIX' survey to 247 practitioners in the US, practitioners spend 4 minutes in average to stop the bleeding during IUD insertion. Using Carevix™, this time can be spared and used for valued patient care.

"Carevix™ is a promising alternative with the potential to dramatically improve the IUD placement experience for women around the world."

Dr. Michal Yaron, Study Investigator, University Hospital of Geneva

Clinical Evidence

Randomized controlled trial data show significantly lower IUD procedural pain and bleeding rates with CarevixTM. Nulliparous women benefited most from the CarevixTM device.²

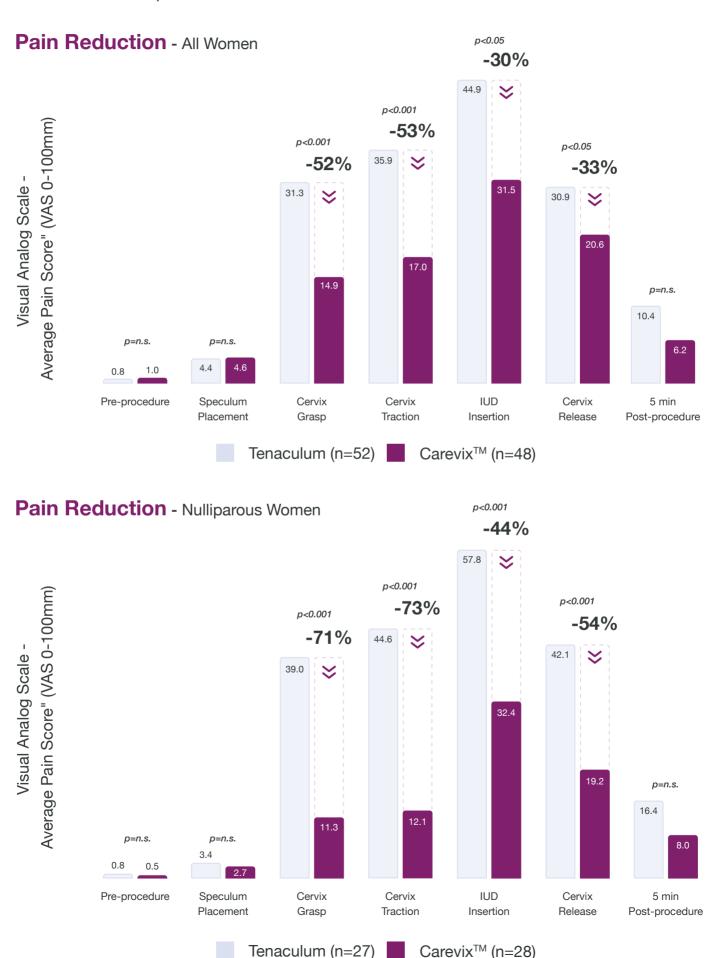

A Novel Approach to Stabilizing the Cervix

Carevix™ is a single-use, suction cervical stabilizer, engineered with vacuum technology, fully designed as a modern alternative to the Tenaculum without compromising on performance.

V

Gentle

Significantly reduces pain and bleeding during cervical engagement while delivering robust traction and maneuverability.¹

Ø

Intuitive

Engineered for ease of use and to mimic current clinical practice requiring minimal learning curve.²

\bigcirc


Versatile

Designed to be used in various transcervical procedures, e.g., IUD, Hysteroscopy, IVF and more. ²



How Carevix™ Works

Components

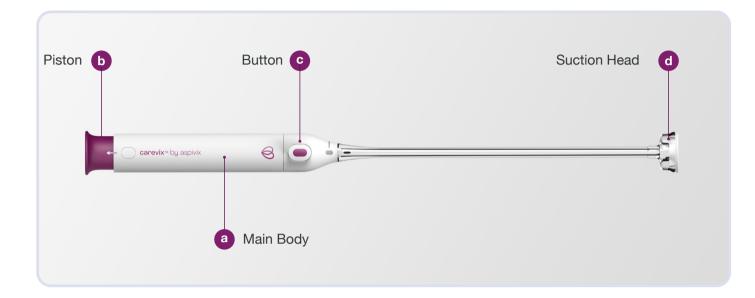

Assembling it



Connect the Suction Head to the Main Body.

Align the connecting marks found on the Suction Head and Main Body Rotate only the Main Body clockwise until it stops and the thin mark on the Main Body is aligned with the thick mark on the Suction Head.

Using Carevix™ - 3 Easy Steps



Pull the Piston to generate the vacuum and rotate to lock it.

to generate the Place the Suction Head on the cervix and press the Button downwards to deliver the vacuum.

Press the Button upwards to release the cervix.

References

- 1. Yaron, M., et al. An Innovative Atraumatic Uterine Cervical Traction Device: A Randomized Trial. Poster presented at: European Society of Contraception and Reproductive Health. Ghent Belgium, May 2022.a
- 2. Aspivix data on file.

Brief Statement

See Instructions for Use for detailed information regarding directions for use and device operations, indications, contraindications, warnings, precautions, and potential adverse events. For further information, contact Aspivix at contact@aspivix.com and/or consult the Aspivix website at www.aspivix.com.



eifu.aspivix.com +800 135 79 135

About Aspivix

We're a medical device start-up from Switzerland. A nimble team of engineers, scientists, gynecologists and seasoned medical technology experts fully devoted to women's healthcare. Our vision at Aspivix is to make Gynecology. Now modern.

ASPIVIX SA
Global Headquarters
Chemin du Closel 5
1020 – Renens
Switzerland



Visit Us

Copyrights ©2022, Aspivix SA. All Rights Reserved. www.aspivix.com

P03-551-001 Rev A ©2022 Aspivix SA. Specifications are subject to change without prior notice. Aspivix, and Carevix are trademarks or registered trademarks of Aspivix SA and/or its subsidiaries. Licensed material is being used for illustrative purposes only. Any person depicted in the licensed material is a model.





Clinically Proven to
Reduce Pain and Bleeding in
Transcervical Procedures

Gentle • Intuitive • Versatile



A Novel Approach to Stabilizing the Cervix

Carevix[™] is a single-use, suction cervical stabilizer, engineered with vacuum technology, fully designed as a modern alternative to the Tenaculum without compromising on performance.

Gentle

Significantly reduces pain and bleeding during cervical engagement while delivering robust traction and maneuverability.¹

Intuitive

Engineered for ease of use and to mimic current clinical practice requiring minimal learning curve.²


Versatile


Designed to be used in various transcervical procedures, e.g., IUD, Hysteroscopy, IVF and more. ²



Clinical Evidence


Randomized controlled trial data show significantly lower IUD procedural pain and bleeding rates with Carevix™. Nulliparous women benefited most from the Carevix™ device.²

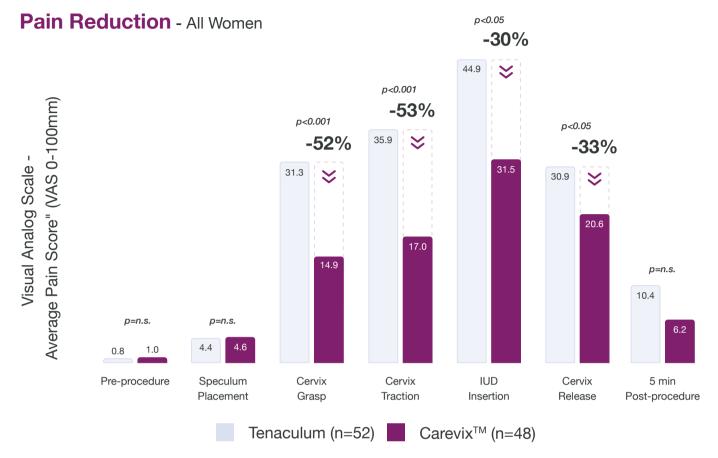

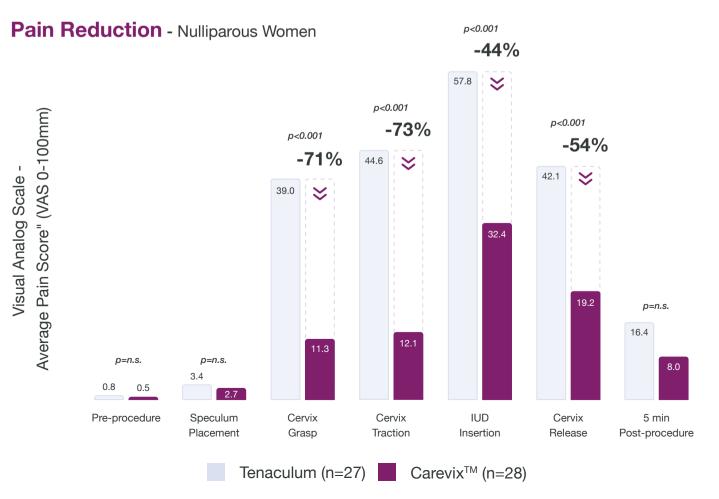

During a clinical study, 100 patients were involved to measure pain experienced during IUD procedures.

Bleeding Results - All Women

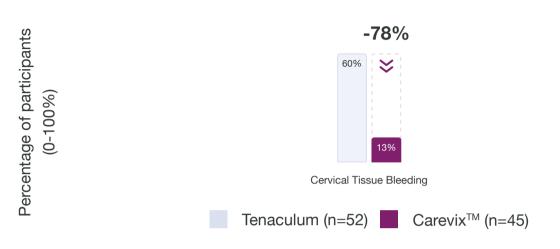

Cervical tissue bleeding frequency is significantly reduced (78% less frequent with Carevix™).

According to ASPIVIX' survey to 247 practitioners in the US, practitioners spend 4 minutes in average to stop the bleeding during IUD insertion. Using Carevix™, this time can be spared and used for valued patient care.

"Carevix™ is a promising alternative with the potential to dramatically improve the IUD placement experience for women around the world."

Dr. Michal Yaron, Study Investigator, University Hospital of Geneva